

UNIVERSIDADE ESTADUAL DE CAMPINAS
SISTEMA DE BIBLIOTECAS DA UNICAMP
REPOSITÓRIO DA PRODUÇÃO CIENTÍFICA E INTELECTUAL DA UNICAMP

Versão do arquivo anexado / Version of attached file:

Versão do Editor / Published Version

Mais informações no site da editora / Further information on publisher's website:

<https://www.nutricionhospitalaria.org/articles/04416/show>

DOI: <https://doi.org/10.20960/nh.04416>

Direitos autorais / Publisher's copyright statement:

©2023 by Aula Médica Ediciones. All rights reserved.

DIRETORIA DE TRATAMENTO DA INFORMAÇÃO

Cidade Universitária Zeferino Vaz Barão Geraldo

CEP 13083-970 – Campinas SP

Fone: (19) 3521-6493

<http://www.repositorio.unicamp.br>



Trabajo Original

Valoración nutricional

Accuracy in body composition scanning by adult half-body DXA scanning

Precisión en la exploración de la composición corporal mediante DXA de medio cuerpo en adultos

Rossana Gómez-Campos¹, Rubén Vidal Espinoza², Ezequiel Moreira Goncalves³, Raquel David Langer³, Juliano Henrique Borges³, Luis Felipe Castelli Correia de Campos⁴, Camilo Urra Alborno⁵, José Sullá Torres⁶, Marco Cossio-Bolaños¹

¹Universidad Católica del Maule. Talca, Chile. ²Universidad Católica Silva Henríquez. Santiago, Chile. ³Universidade Estadual de Campinas – UNICAMP. São Paulo, SP, Brazil.

⁴Universidad del Bío Bío. Chillán, Chile. ⁵Universidad Autónoma de Chile. Chile. ⁶Universidad Católica de Santa María. Arequipa, Perú

Abstract

Introduction: dual-energy X-ray absorptiometry (DXA) is the gold standard method, although one limitation is the size of the scan area.

Objective: the objective was to verify the accuracy of body composition (BC) scanning through half-body DXA scanning compared to standard total body scanning.

Methods: a study was conducted on 145 volunteers. Weight and height were assessed. Body mass index (BMI) was calculated. DXA was used for whole-body scan (WBS) and half-body scan (HBS). WBS was used as the reference method and the following indicators were extracted: bone mineral content (BMC), fat mass (FM), lean soft tissue (LST) and percentage fat mass (%FM).

Results: no differences were observed in the body composition indicators (BMC, FM, LST and %FM) when compared between the reference WBS scanner and the HBS scanner. The predictive power between both scans ranged in both sexes between $R^2 = 0.94$ and 0.98 . The DRI desirable reproducibility index values defining the degree of agreement between both scans ranged from 0.97 to 0.99 , and the values for precision (0.97 to 0.99) and accuracy (0.99) were high.

Conclusion: HBS scanning by DXA evidenced agreement, and high values of accuracy and precision to assess body composition indicators (BMC, FM, LST and %FM).

Keywords:

DXA. Body composition.
Accuracy. Adult.

Resumen

Introducción: la absorciometría de rayos X de doble energía (DXA) es el método de referencia, aunque una limitación es el tamaño del área de exploración.

Objetivo: el objetivo fue verificar la precisión de la exploración de la CB mediante la exploración DXA de medio cuerpo en comparación con la exploración estándar de todo el cuerpo.

Métodos: se realizó un estudio con 145 voluntarios. Se evaluaron el peso y la altura. Se calculó el índice de masa corporal (IMC). Se utilizó la DXA para la exploración de cuerpo entero (WBS) y la exploración de medio cuerpo (HBS). Se utilizó la PEP como método de referencia y se extrajeron los siguientes indicadores: contenido mineral óseo (CMO), masa grasa (MG), tejido blando magro (TBL) y porcentaje de masa grasa (%MG).

Resultados: no se observaron diferencias en los indicadores de composición corporal (BMC, FM, LST y %FM) cuando se compararon entre el escáner WBS de referencia y el escáner HBS. El poder predictivo entre ambos escáneres osciló en ambos sexos entre $R^2 = 0,94$ y $0,98$. Los valores del índice de reproducibilidad deseable DRI que definen el grado de acuerdo entre ambas exploraciones oscilaron entre $0,97$ y $0,99$, y los valores de precisión ($0,97$ a $0,99$) y exactitud ($0,99$) fueron altos.

Conclusión: la exploración de HBS mediante DXA evidenció concordancia y altos valores de exactitud y precisión para evaluar los indicadores de composición corporal (BMC, FM, LST y %FM).

Palabras clave:

DXA. Composición corporal.
Precisión. Adulto.

Received: 28/08/2022 • Accepted: 11/12/2022

Conflicts of interest: the authors declare none.

Gómez-Campos R, Vidal Espinoza R, Moreira Goncalves E, David Langer R, Borges JH, Castelli Correia de Campos LF, Urra Alborno C, Sullá Torres J, Cossio-Bolaños M. Accuracy in body composition scanning by adult half-body DXA scanning. Nutr Hosp 2023;40(2):362-367

DOI: <http://dx.doi.org/10.20960/nh.04416>

Correspondence:

Rossana Gómez-Campos. Universidad Católica del Maule. Av. San Miguel 3605. Talca, Chile
e-mail: rossaunicamp@gmail.com

INTRODUCTION

Dual-energy X-ray absorptiometry (DXA) is an accurate method for measuring total body and subregional bone mineral density (BMD), bone mineral content (BMC), fat mass (FM), and lean soft tissue (LST) (1-3). This method has the advantage of a short scan time (5-20 min) (4) and a low radiation dosage ($\pm 10 \mu\text{Sv}$) (5). Moreover, it can be used with children and adolescents (6,7).

The three major commercial manufacturers of DXA are GE Medical Systems Inc. (formerly Lunar), Madison, WI, USA; Hologic Inc., Waltham, MA, USA; and Cooper-Surgical (formerly Norland Medical Systems, Inc.), Trumbull, CT, USA (8,9). One of the limitations of DXA is the size of the active scanning area. DXA machines have dimensions of approximately 60-67 cm in width and 193-198 cm in length (8,9).

The width of the scanning area can compromise the accuracy of the measurement when body dimensions exceed these limits. This is also true for people with a large trunk and skeletal muscle mass favorable for particular sports, such as bodybuilding, rowing, and rugby or obese patients (9), although currently new equipment can assess an area of 228 cm in length, 137 cm in width and a weight of 280 kg (7). However, these devices are not always available in laboratories, so in order to solve this methodological limitation, some researchers have studied the accuracy of half-body scans using DXA (HBS) for estimating the whole-body composition (10,11).

Indeed, some studies measured body composition by DXA in obese adults (4,12), obese children (7,13) and physically active young adults (11). Thus, analysis of the accuracy and homogeneity of half-body scans can improve the applicability of the technique in a clinical context (7), mainly when a person's body dimensions exceed these limits and even in patients with metallic implants in their extremities (14).

In general, to our knowledge, a study of this nature was not performed in the Chilean population, so this information could be relevant when evaluating heterogeneous adult populations.

Therefore, the aim of the study was, to verify the accuracy in body composition scanning through the half-body DXA scan compared to the standard total body scan, using GE Lunar Prodigy DXA

The data collection process was carried out in a laboratory of the Autonomous University between April and July 2019 from Monday to Friday from 8:30 am to 12:30 pm. The study was approved by the Research Ethics Committee of the local university.

INSTRUMENTATION

The anthropometric variables of weight and height were evaluated following the recommendations of Ross, Marfell-Jones (15). Body weight (kg) was assessed with a scale (SECA, Hamburg, Germany) accurate to 0.1 kg. Standing height was measured with a stadiometer (SECA, Hamburg, Germany) to the nearest 0.1 cm. BMI was calculated by means of the formula $[\text{BMI} = \text{weight (kg)} / \text{height (m)}^2]$.

Two DXA scans were performed the same day for analysis. First, WBS was performed and used as a reference. Second, HBS was performed to estimate the whole-body composition to compare it with the reference method. The same technician positioned the subjects, performed the three scans, and executed the analysis according to the operator's manual using the standard analysis protocol. Standardized positioning was maintained during HBS with volunteers in a supine position with the left sagittal line of scan window under the left upper limb. Right half-body composition was used to estimate the whole-body composition. Subjects were warned not to wear jewelry and to avoid the presence of any type of metal on the body that could impede scanning.

DUAL ENERGY X-RAY ABSORPTIOMETRY (DXA)

DXA measurements were taken using a total-body scanner (Lunar Prodigy; GE Healthcare, Madison, WI, USA). The Lunar Prodigy DXA is an instrument with a weight limit of 160 kg and a relatively large space exploration of 197.5 x 66 cm. Scan analysis was performed using GE Encore 11.10 software (GE, Madison, WI, USA). The following variables were extracted from the DXA software: bone mineral content (BMC), fat mass (FM), Lean soft tissue (LST) and fat mass percentage %FM. The DXA was calibrated each day before measurement according to the manufacturer's guidelines. The coefficients of variation (CV) in our laboratory were 1.4 %, 1.6 %, and 1.0 % for BMC, FM, and LST, respectively.

STATISTICAL ANALYSIS

A descriptive analysis (mean \pm standard deviation [SD], minimum and maximum), and the Kolmogorov-Smirnov test for normality were performed. We used Student's paired t-test to compare Pearson's correlation coefficient (r) to verify the relationship between the variables and linear regression analysis (adjusted coefficient of determination $[R^2]$). Additionally, the standard error of estimate [SEE] was used to verify explanation power of HBS in estimating the whole-body composition with WBC. The concor-

MATERIALS AND METHODS

SUBJECTS

A cross-sectional study was carried out on 145 volunteers (62 males and 83 females) between 18 and 70 years of age to compose the sample. Subjects fitting into the scanning area (197.5 x 66) of GE Lunar Prodigy were eligible to participate in the study. Those who did not complete the evaluations and those who presented some type of physical disability that prevented them from moving on their own were excluded. All volunteers were informed of the objective of the study and subsequently signed and authorized the informed consent form.

dance correlation coefficient (CCC) proposed by Lawrence, Lin (16) was also calculated to verify precision and accuracy. The significance level was set at $\alpha \leq 0.05$. The SPSS version 16.0 (IBM Corp., Armonk, NY, USA) was used for the statistical analysis, as well as MedCalc 11.1.0.

RESULTS

The anthropometric variables characterizing the sample studied can be seen in table I. There were no significant differences in age ($p = 0.23$) and BMI ($p = 0.74$) between both sexes. However, as expected, men presented higher weight and height in relation to women ($p < 0.000$).

Comparisons of BMC, FM, LST and %FM values between total body and half body by sex are shown in table II. There were no significant differences between both scans ($p = 0.81$ to 0.99) in both men and women.

The correlations between both scans according to body composition indicators are shown in figure 1. In men and in the four indicators (BMC, FM, LST and %FM) the predictive power ranged from $R^2 = 0.94$ to 0.98 . For women the values explained from $R^2 = 0.96$ to 0.98 , respectively.

The DRI values that define the degree of agreement between both scans are shown in table III. In general, it is observed that the half-body scan shows a CCC with the reference method (total body) from 0.97 to 0.99 . In addition, the values of precision (0.97 to 0.99) and accuracy (0.99) in both sexes are high.

Table I. Characteristics of the sample studied

Variables	Males (n = 62)		Females (n = 83)		t	p
	X	SD	X	SD		
Age (years)	51.9	21.9	55.8	17.4	-1.230	0.223
Weight (kg)	77.8	14.4	67.0	14.0	4.540	0.000
Height (cm)	169.2	7.4	154.3	11.5	8.930	0.000
BMI (kg/m ²)	27.2	4.5	27.4	4.2	-0.330	0.746

X: mean; SD: standard deviation; BMI: body mass index.

Table II. Comparison of total-body and half-body composition indicators in both sexes

Indicators	Whole-body scan		Half-body scan		p
	X	SD	X	SD	
Males					
BMC (kg)	2.87	0.41	2.87	0.39	0.999
FM (kg)	21.01	8.62	21.09	8.66	0.959
LST (kg)	56.67	8.39	56.4	8.35	0.849
%FM	26.36	7.32	26.54	7.26	0.891
Females					
BMC (kg)	2.07	0.33	2.09	0.7	0.814
FM (kg)	25.93	7.3	26.03	7.53	0.931
LST (kg)	40.15	5.07	40.06	5.23	0.911
%FM	38.68	6.59	38.79	6.74	0.916

X: mean; SD: standard deviation; BMC: bone mineral content; FM: fat mass; LST: lean soft tissue; %FM: percentage of fat mass.

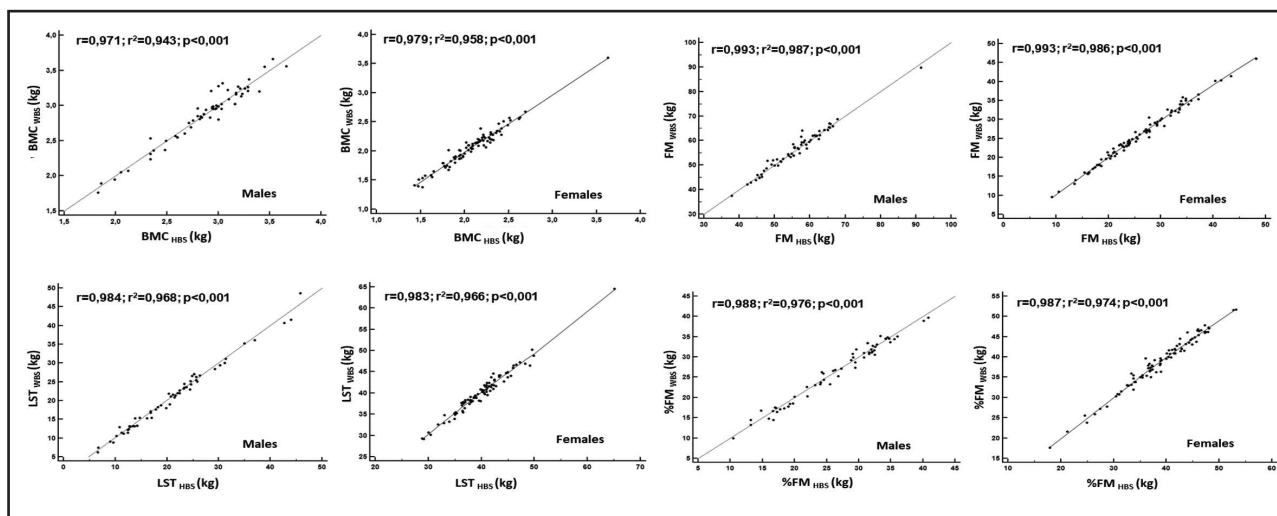


Figure 1.

Relationship between both scans (total body and half body) according to body composition indicators in both sexes.

Table III. Desirable reproducibility index (DRI) values to define the agreement between total body and half body DXA scans

Indicators	X	SD	CCC	Precision	Accuracy
Males					
BMC (TB)	2.87	0.41	--	--	--
BMC (HB)	2.87	0.39	0.97	0.97	0.99
FM (TB)	21.01	8.61	--	--	--
FM (HB)	21.09	8.65	0.99	0.99	0.99
LST (TB)	56.67	8.39	--	--	--
LST (HB)	56.4	8.34	0.98	0.98	0.99
%FM (TB)	26.36	7.32	--	--	--
%FM (HB)	26.54	7.26	0.98	0.98	0.99
Females					
BMC (TB)	2.07	0.33	--	--	--
BMC (HB)	2.09	0.33	0.97	0.98	0.99
FM (TB)	25.93	7.3	--	--	--
FM (HB)	26.03	7.53	0.99	0.99	0.99
LST (TB)	40.15	5.07	--	--	--
LST (HB)	40.06	5.23	0.98	0.98	0.99
%FM (TB)	38.68	6.59	--	--	--
%FM (HB)	38.79	6.74	0.98	0.98	0.99

X: mean; SD: standard deviation; CCC: concordance correlation coefficient; BMC: bone mineral content; FM: fat mass; LST: lean soft tissue; %FM: percentage of fat mass.

DISCUSSION

The aim of the study was to verify the accuracy of body composition scanning through HBS DXA scanning compared to standard WBS scanning, using GE Lunar Prodigy DXA.

The results of the study have shown that the half-body scan reflects similar results as the total body scan in the indicators of BMC, FM, LST and %FM. These findings are consistent with some studies that compared both methods (4,7,10,12).

In fact, no bias was observed in the results, even the correlations between both methods were high and almost perfect, ranging from 0.93 to 0.99 as reported by other studies (7,17).

Evidently, HBS scanning has reflected wide concordance and precise and accurate values versus WBS scanning, as this information allows highlighting that the HBS scanning technique supports the use of DXA to scan a larger number of subjects and in less time. It also allows the inclusion of those subjects that are outside the scanning area (7) due to their extreme body dimensions (9).

In fact, DXA has become a popular tool for measuring body composition due to its ease of operation, completeness of analysis and gold standard (18,19). For nowadays WBS and HBS scanning, can be considered as precise and accurate scanning techniques, moreover, some studies have used HBS scanning to predict body composition in weight reduction programs in obese patients who barely fit in the scanning area (20) and even, to verify body composition changes after bariatric surgery in morbidly obese individuals (21).

In that sense, it is important that studies develop a satisfactory technique to scan individuals of all physical types (11), these include patients who present metallic implants in their extremities, as they are often excluded from studies covering body composition analysis (15).

Also, it is widely known that most manufacturers' manuals do not verify the use of DXA for body composition analysis in subjects with a metallic implant (22).

Consequently, having the HBS scanning technique in clinical and epidemiological contexts may avoid excluding some patients who are likely to have extreme physical characteristics, as well as amputations and/or metallic implants in some of their extremities. On the contrary, HBS scanning opens new perspectives and possibilities to be implemented in clinics and laboratories to cover not only conventional but also non-conventional populations.

In general, DXA is a non-invasive, fast, safe and low radiation method equivalent to a day sunbathing (23), in addition, in recent years, DXA equipment have been improving over time in their designs and manufacturing models, for example, they have been reducing scanning times, as well as have ostensibly improved the quality in their images in terms of pixels (24).

This research presents some strengths, given that it is the first study that verified the applicability of the use of HBS scanning in a sample of Chilean adults. In addition, the results obtained in this study can serve for future comparisons, as well as a baseline to verify trends among the adults studied.

Notwithstanding the above, the study has some limitations, for example, the type of sample selection and the number of

participants considered were not large enough. These aspects could limit the generalizability of the results to other contexts, so they should be analyzed with caution. Future studies should consider the use of more sophisticated equipment to corroborate our findings.

In conclusion, this study demonstrated that HBS scanning through DXA evidenced concordance and high values of precision and accuracy to assess body composition indicators (BMC, FM, LST and %FM.) in adult patients. The results suggest the use and application in research, clinical and epidemiological contexts.

REFERENCES

1. Fan B, Shepherd JA, Levine MA, Steinberg D, Wacker W, Barden HS, et al. National Health and Nutrition Examination Survey whole-body dual-energy X-ray absorptiometry reference data for GE Lunar systems. *J Clin Densitom* 2014;17(3):344-77. DOI: 10.1016/j.jocd.2013.08.019
2. Powers C, Fan B, Borrud LG, Looker AC, Shepherd JA. Long-term precision of dual-energy X-ray absorptiometry body composition measurements and association with their covariates. *J Clin Densitom* 2015;18(1):76-85. DOI: 10.1016/j.jocd.2013.09.010
3. Kutáč P, Bunc V, Sigmund M. Whole-body dual-energy X-ray absorptiometry demonstrates better reliability than segmental body composition analysis in college-aged students. *PLoS One* 2019;14(4):e0215599. DOI: 10.1371/journal.pone.0215599
4. Rothney MP, Brychta RJ, Schaefer EV, Chen KY, Skarulis MC. Body composition measured by dual-energy X-ray absorptiometry half-body scans in obese adults. *Obesity (Silver Spring)* 2009;17(6):1281-6. DOI: 10.1038/oby.2009.14
5. Blake GM, Naeem M, Boutros M. Comparison of effective dose to children and adults from dual X-ray absorptiometry examinations. *Bone* 2006;38(6):935-42. DOI: 10.1016/j.bone.2005.11.007
6. Rodrigopulle DJ, Atkinson SA. Validation of surrogate limb analysis for body composition in children by dual energy X-ray absorptiometry (DXA). *Eur J Clin Nutr* 2014;68(6):653-7. DOI: 10.1038/ejcn.2014.44
7. Ferreira MS, Marson FAL, Wolf VLW, da Silva MTN, Zambon MP, Antonio MARGM, et al. Concordance between whole- and half-body scans to evaluate body composition in dual-energy X-ray absorptiometry in children and adolescents with different nutritional and pubertal conditions. *Nutrition* 2019;66:78-86. DOI: 10.1016/j.nut.2019.03.018
8. Brownbill RA, Ilich JZ. Measuring body composition in overweight individuals by dual energy x-ray absorptiometry. *BMC Med Imaging* 2005;5(1):1. DOI: 10.1186/1471-2342-5-1
9. Silva AM, Heymsfield SB, Sardinha LB. Assessing body composition in taller or broader individuals using dual-energy X-ray absorptiometry: a systematic review. *Eur J Clin Nutr* 2013;67(10):1012-21. DOI: 10.1038/ejcn.2013.148
10. Breithaupt P, Colley RC, Adamo KB. Body composition measured by dual-energy X-ray absorptiometry half-body scans in obese children. *Acta Paediatr* 2011;100(12):e260-6. DOI: 10.1111/j.1651-2227.2011.02378.x
11. Nana A, Slater GJ, Hopkins WG, Burke LM. Techniques for undertaking dual-energy X-ray absorptiometry whole-body scans to estimate body composition in tall and/or broad subjects. *Int J Sport Nutr Exerc Metab* 2012;22(5):313-22. DOI: 10.1123/ijnsnem.22.5.313
12. Tataranni PA, Ravussin E. Use of dual-energy X-ray absorptiometry in obese individuals. *Am J Clin Nutr* 1995;62(4):730-4. DOI: 10.1093/ajcn/62.4.730
13. Breithaupt P, Colley RC, Adamo KB. Body composition measured by dual-energy X-ray absorptiometry half-body scans in obese children. *Acta Paediatr* 2011;100(12):e260-6. DOI: 10.1111/j.1651-2227.2011.02378.x
14. Hsiao PL, Hsu SF, Chen PH, Tsai HW, Lu HY, Wang YS, et al. Does a spinal implant alter dual energy X-ray absorptiometry body composition measurements? *PLoS One* 2019;14(9):e0222758. DOI: 10.1371/journal.pone.0222758
15. Ross WD, Marfell-Jones MJ. *Kinanthropometry. Physiological Testing of Elite Athlete. Human Kinetics: Champaign, IL, USA; 1991.* pp. 223-308
16. Lin LI. A concordance correlation coefficient to evaluate reproducibility. *Biometrics* 1989;45(1):255-68.

17. Evans EM, Prior BM, Modlesky CM. A mathematical method to estimate body composition in tall individuals using DXA. *Med Sci Sports Exerc* 2005;37(7):1211-5. DOI: 10.1249/01.mss.0000170077.87301.65
18. Bazzocchi A, Ponti F, Diano D, Amadori M, Albisinni U, Battista G, et al. Trabecular bone score in healthy ageing. *Br J Radiol* 2015;88(1052):20140865. DOI: 10.1259/bjr.20140865
19. de Silva MHAD, Hewawasam RP, Lekamwasam S. Concordance between Body Composition Indices Measured with Dual-Energy X-Ray Absorptiometry and Bioelectrical Impedance Analysis in Obese Children in Sri Lanka. *Int J Pediatr* 2021;2021:6638057. DOI: 10.1155/2021/6638057
20. Lundqvist K, Neovius M, Grigorenko A, Nordenstroem J, Roessner S. Use of dual-energy X-ray absorptiometry in obese individuals: The possibility to estimate whole body composition from DXA half-body scans. *Radiography* 2009;15(1):12-9. DOI: 10.1016/j.radi.2008.02.006
21. Levitt DG, Beckman LM, Mager JR, Valentine B, Sibley SD, Beckman TR, et al. Comparison of DXA and water measurements of body fat following gastric bypass surgery and a physiological model of body water, fat, and muscle composition. *J Appl Physiol* (1985) 2010;109(3):786-95. DOI: 10.1152/japplphysiol.00278.2010
22. Di Monaco M, Vallero F, Di Monaco R, Tappero R. Prevalence of sarcopenia and its association with osteoporosis in 313 older women following a hip fracture. *Arch Gerontol Geriatr* 2011;52(1):71-4. DOI: 10.1016/j.archger.2010.02.002
23. Ponti F, Santoro A, Mercatelli D, Gasperini C, Conte M, Martucci M, et al. Aging and Imaging Assessment of Body Composition: From Fat to Facts. *Front Endocrinol (Lausanne)* 2020;10:861. DOI: 10.3389/fendo.2019.00861
24. Watson LPE, Venables MC, Murgatroyd PR. An Investigation Into the Differences in Bone Density and Body Composition Measurements Between 2 GE Lunar Densitometers and Their Comparison to a 4-Component Model. *J Clin Densitom* 2017;20(4):498-506. DOI: 10.1016/j.jocd.2017.06.029